# MODE D'EMPLOI : STERILISATEUR DOUBLE FONCTION

## UTILISATION A CHAUD : MICRO-ONDES

**1)** Verser 100 ml d'eau du robinet dans le récipient de base.
Vous pouvez utiliser un biberon gradué pour mesurer cette quantité.

**2)** Lavez et rincez soigneusement les biberons et accessoires.

**3)** Posez la grille dans le récipient de base dans le sens indiqué sur le schéma puis insérer les biberons (4 au maximum) et accessoires dans le bac.

**4)** Fermer le stérilisateur avec le couvercle puis placer l'ensemble de stérilisation au centre micro-ondes.

**5)** Régler le four micro-ondes sur la puissance **500 watts Maxi.**
Faire chauffer **5 minutes Maxi.**

☞ **EN CAS DE DEPASSEMENT DE CES VALEURS, RISQUE DE DETERIORATION DES BIBERONS ET DU STERILISATEUR.**

**6)** Le temps de stérilisation écoulé, **attendre au moins 3 minutes avant de sortir le stérilisateur** du micro-ondes.

**7)** Lorsque l'appareil a suffisamment refroidi, retirer le couvercle avec précaution et laisser la vapeur s'échapper. Tous les éléments sont prêts à l'emploi.

**ATTENTION :**

- Pour les biberons de grande taille, veillez à ce qu'ils n'empêchent pas la fermeture du couvercle.
- Après chaque utilisation, vider le stérilisateur.
- Placer le stérilisateur loin d'une source de chaleur et hors de portée des enfants.
- Bien respecter le volume d'eau indiqué pour la stérilisation.
- **Ne pas faire fonctionner l'appareil sans eau**.
  ☞ **N'INTRODUIRE NI SOLUTION, NI PASTILLE CHIMIQUE DANS LE STERILISATEUR EN FONCTIONNEMENT MICRO ONDES.**
- Pour les fours mixtes, s'assurer avant utilisation que le grill n'est pas actionné et que le four n'est pas chaud. Pour plus de précisions sur le réglage de votre four micro-ondes, reportez-vous à la notice du fabricant.
- **Vérifier la température du récipient de base avant de le sortir du four micro-ondes. Le manipuler avec précaution car il contient de l'eau très chaude et de la vapeur. Ne pas approcher votre visage en ouvrant le couvercle.**

- Ne pas utiliser ce stérilisateur pour les goupillons, les jouets et anneaux de dentition, ainsi que les objets en métal.

Vérifier toujours la température de la nourriture avant de nourrir bébé.

100 ml d'eau du robinet

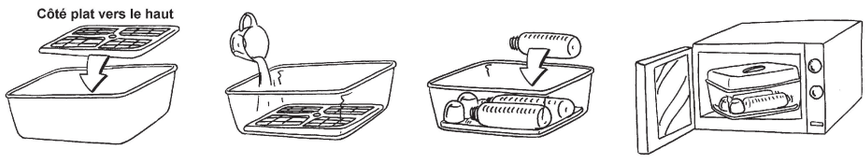


## UTILISATION A FROID : COMPRIMES DE STERILISATION

1) Après utilisation, bien nettoyer les biberons et accessoires à l'aide d'un goupillon.
2) Remplir le bac avec de l'eau du robinet.
3) Ajouter 1 comprimé de stérilisation pour 2 ou 3 litres d'eau.
4) Après dissolution des comprimés, immerger complètement biberons et accessoires dans la solution. Il ne doit pas rester d'air dans les biberons.
5) Apposer la grille pour assurer l'immersion des biberons et accessoires. Poser le couvercle.
6) En 30 minutes, les biberons et accessoires sont stérilisés.
7) Rincer à l'eau minérale, biberons et accessoires avant utilisation.

La solution reste stérile pendant 24 heures. Il est donc préférable d'y laisser tous les éléments jusqu'à leur utilisation.
En cours de journée, vous pouvez y ajouter d'autres biberons et accessoires.
Passé le délai de 24 heures, il faut renouveler la solution.

**ATTENTION :**

- Tenir les comprimés et la solution hors de portée des enfants.
- Ne jamais mettre d'objets métalliques dans la solution.
- Eviter tout contact avec les yeux.
- Les comprimés et la solution ne doivent pas être avalés – En cas d'absorption, contacter immédiatement un médecin.
- Ne pas rajouter d'autre produit dans la solution.
- Manipuler avec précaution, car les comprimés ou la solution peuvent provoquer une décoloration des tissus.
- L'évacuation de la solution de stérilisation à froid n'est pas nuisible pour les fosses septiques.
- Utiliser de préférence les comprimés de stérilisation THERMOBABY.

## MODE D'EMPLOI DU STERILISATEUR DOUBLE EMPLOI

A lire attentivement et à conserver pour consultation ultérieure.

*Thermobaby – Z.I. de Kerbois – 56400 AURAY France –*
*tel : (33) 02 97 24 11 66 – fax : (33) 02 97 24 16 17*
http://www.thermobaby.com – *e-mail :* com@thermobaby.com

# INSTRUCTION FOR USE : DUAL FUNCTION STERILIZER

## HOT USE : MICRAWE OWEN

1) Pour 100ml of tap water in the container.
   You can use a feeding bottle to measure this quantity.
2) After each use, clean the feeding bottles and accessories thoroughly.
3) Put the rack in the container.
   Put the feeding bottles (4 is a maximum) and accessories on the rack.
4) Close the microwave steriliser with the lid and put it in the middle of your microwave oven.
5) Select the power **500 watts Maxi.**
   Sterilisation takes **5 minutes Maxi.**

   ☞ **FAILURE TO RESPECT THESE INSTRUCTIONS COULD LEAD TO DAMAGE BOTH FEEDING BOTTLES AND STERILISER.**
6) When the time required for sterilisation is over, let the steriliser cool down for at least 3 minutes before taking it out of the microwave oven.
7) When the steriliser cools down enough, take out the lid carefully and let the steam escapes. The feeding bottles and accessories are ready for use.

**SAFETY MEASURES :**

- For big feeding bottles, check that they do not obstruct the perfect closing of the steriliser.
- Empty the steriliser after each use.
- Keep the steriliser in a safe and stable place, out of the reach of children.
- Do not place the steriliser near an open flame or a hot surface.
- Always use the correct quantity of tap water as stipulated in those instructions. Never use the steriliser without water.
  ☞ **DO NOT INSERT NEITHER CHEMICAL SOLUTIONS NOR TABLETS IN THE STERILISER WHEN IT IS USED IN MICROWAVE OVEN.**
- Check that your microwave oven is not hot before introducing the microwave steriliser.
- Let the microwave steriliser cool down before taking it out of the microwave oven.
- **Be very careful when you take it out of the microwave oven as the steriliser contains very hot water and steam.**
- **Be very careful when the steam escapes from the steriliser.**
- Do not use this microwave steriliser for bottle brushes, toys and teething ring, neither for metallic products.

100 ml of tap water

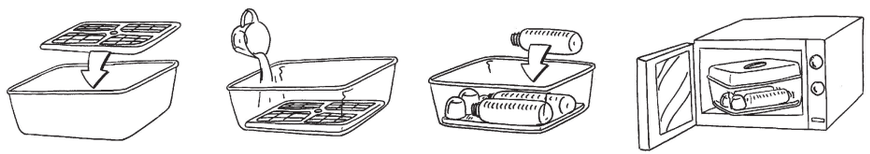

## COLD USE : STERILIATION TABLETS

1) After use, clean the feeding-bottles and accessories thoroughly with a bottle-brush.
2) Fill the container with tap water.
3) Add 1 sterilisation tablet for 2 or 3 litres.
4) After the tablets have dissolved, immerse feeding-bottles and accessories completely in the solution. Here must be no air left in the bottle.
5) Position the grid to ensure complete immersion of bottles and accessories. Cover with the lid.
6) After 30 minutes, the bottles and accessories are sterilised.
7) Rinse both bottles and accessories in mineral water before use.

The solution remains sterile before 24 hours. Therefore it is best to leave all elements in it until they are required.
Throughout the day, you can add other bottle and accessories.
But beyond the 24 hours limit, it is essential to change the solution.

**SAFETY MEASURES :**

- Keep the tablets and solution out of the reach of children.
- Never keep metallic objects in the solution.
- Avoid all contact with the eyes.
- Do not swallow the tablet or solution – In this event, call a doctor immediately.
- Do not add any other product to the solution.
- Handle with care, since the tablets or the solution may discolour fabrics.
- The cold sterilisation solution can be disposed of to a septic tank.
- We recommend the use of THERMOBABY stérilisation tablets.

**INSTRUCTION FOR USE : DUAL FUNCTION STERILIZER**
To be read carefully and conserved

*Thermobaby – Z.I. de Kerbois – 56400 AURAY France –*
*tel : (33) 02 97 24 11 66 – fax : (33) 02 97 24 16 17*
http://www.thermobaby.com – *e-mail :* com@thermobaby.com